

수정진동자를 이용한 결정성장의 측정

김병철, 강현욱, 정수영, 김영한*
동아대학교 화학공학과
(yhkim@mail.donga.ac.kr*)

Measurement of Crystal Growth with a Quartz Crystal Oscillator

Byoung Chul Kim, Hyun Woog Kang, Su Yeong Jeong and Young Han Kim*
Dept. of Chemical Engineering, Dong-A University
(yhkim@mail.donga.ac.kr*)

INTRODUCTION

The shape of crystallization product is a key factor to control crystallization processes, because the shape determines the product quality. The shape disparity often incurs large difference in the product price. Though the product shape and growth are controlled by the introduction time of seed crystals and the temperature adjustment of crystallization solution in cooling crystallization, the control for a desired crystal shape largely depends upon the experience of an operator. It is because the measurement of solution state is difficult for the prediction of the product shape. In practice, the solution concentration and temperature are measured to determine the seed introduction moment and the cooling rate of solution, but the accurate determination is not simple because a small error in the concentration and temperature measurements leads to a large difference of the product quality.

A direct monitoring system of the crystallization processes using an inter digital transducer (IDT) and a surface acoustic wave (SAW) sensor was introduced. By lowering temperature of the sensor surface, a cooling crystallization of sample solution was induced to form crystals on the surface and to reduce the wave frequency of the sensor. The frequency decrease is proportional to the crystal mass formed on the sensor surface, which can be utilized in the temperature control of the crystallization solution. Similarly, a quartz crystal oscillator has been widely used owing to its size and simplicity of the measurement in the determination of nano-scale variation of mass and rheological property of a thin film contacting to the oscillator surface. The quartz crystal oscillator has also been implemented in the monitoring of crystal formation at the beginning stage of cooling crystallization processes [1-3].

In this study, the monitoring system of the quartz crystal oscillator was employed in the prediction of crystal shape from two crystallization processes of potassium nitrate and cupric sulfate. A controlled cooling crystallization was induced on the oscillator surface, and the frequency variation was measured and compared with the result of microscopic observation of produced crystals. From the experimental outcome, the availability of the crystal shape prediction using the oscillator system was examined here.

EXPERIMENTAL

Two rooms of salt solution and cooling ethanol were separated with a quartz crystal oscillator, and two polyethylene plates and two o-rings were used to build a room on each side of the oscillator. Two pumps provided separate flows of saturated salt solution and cooling ethanol to the rooms. The plates were square, and their thicknesses were 3 mm for inner side and 5 mm for outer side. An AT-cut quartz crystal oscillator having a base frequency of 8 MHz (Sunny Electronics Co., Korea) was utilized in this experiment. The electrode of the crystal was silver finished. The oscillator was placed in vertical position in order to prevent the sedimentation of floating crystals and foreign suspended particles.

Two sets of temperature control and liquid circulation systems for salt solution and coolant were installed in the experimental apparatus as shown in Figure 1. The oscillator module located in the middle of the setup and the salt solution was fed from the left hand side, and the coolant was provided from the right. Two thermostats were utilized for the control of temperatures of the

solution and coolant. For fast manipulation of coolant temperature a glass heat exchanger was used, and a water containing thermostat supplied temperature adjusted water to the heat exchanger. The temperature of cooling ethanol was manipulated by the water temperature. The temperature of the thermostat was controlled with a programmable temperature controller.

An oscillation circuit contained in the box beneath the sensor module was directly connected to the quartz crystal oscillator to prevent possible weakening of the electric signal from the oscillator. Temperatures of the salt solution and coolant were measured with a tiny platinum resistance thermometer of 0.9 mm in diameter and 15 mm long (Konics Instrument, Korea, Model C100/09158). The oscillation frequency was counted using a home-made frequency counter, and resonant resistance was measured with a built-in amplifier in the counter. The digital signals of resonant frequency and resonant resistance were provided to a PC for data processing.

Two salts, potassium nitrate (Katayam Chemical, Japan, Code No. 24-5020) and cupric sulfate (Shinyo Pure Chemicals, Japan, 1st grade) were used as received in this experiment. Ethanol (Hayman, U. K., Code No. 200-578-6) were utilized as a coolant.

An 11.7 g of potassium nitrate was dissolved into distilled water of 300 mL contained in a 500 mL glass bottle to the saturated concentration at a temperature of 25 °C. The bottle was placed in a thermostat to be maintained at the temperature. The sensor module was assembled, and the electric wires were connected to make the signal steady. A bottle of cooling ethanol was prepared, and the ethanol was pumped to the glass heat exchanger. The water from the other thermostat was supplied to the heat exchanger with a pump. The temperature adjusted ethanol from the exchanger was supplied to the sensor module at a flow rate of 7 mL/min after half an hour settlement of the sensor module. When the oscillation frequency was steady, the saturated potassium nitrate solution was provided to the left hand side of the sensor module at a rate of 7 mL/min. When the oscillation frequency was stable again, the programmable temperature controller for coolant temperature adjustment was activated and the measurements of resonant frequency and resistance was initiated. The manipulation of coolant temperature was determined at the beginning of the experiment, and the resonant frequency and resistance, and the temperatures of solution and coolant were stored in a PC for the analysis of experimental result. The experiment was conducted again with cupric sulfate using the same procedure that explained above.

After the experiment the sensor module was disassembled to take out the oscillator with crystals on it for the observation of crystal shape. The oscillator surface was carefully rinsed with ethanol, and dried to observe the surface with a scanning electron microscope (Hitachi High-Technologies, Japan, Model S-2400). In cases of experimental run-1 and run-2, the produced crystal was dissolved to inspect the oscillator stability by checking the initial frequency and resistance. Therefore, the same experiment of crystal production was conducted again to obtain the oscillator with the crystal. The cooling rate was adjusted at the same as the frequency measurement until sufficient crystals were made on the oscillator, which was taken for the microscopic observation.

RESULTS AND DISCUSSION

The variations of resonant frequency and resistance are shown in top two figures of Figure 2. While the temperature of potassium nitrate solution was maintained at the same, the coolant temperature was reduced to induce the crystal formation and raised to dissolve the crystal. The frequency decrease indicates the crystal formation, and the elevation of resonant resistance demonstrates the increase of surface roughness due to the formation. As the crystals dissolve, the frequency and resistance return to the initial values. The cooling rate and frequency dropping rate are listed in Table 1. A similar experiment was conducted with higher rate of coolant temperature variation, and the outcome is described.

One can predict that a slow cooling crystallization of salt solution produces crystals of its intrinsic shape, but the critical cooling rate is hard to determine. By monitoring the resonant frequency variation of a quartz crystal oscillator the crystallization rate can be determined because the frequency reduction is proportional to the mass increase of the crystals produced. To compare the crystallization

product of potassium nitrate in two different rates of cooling, the cooling crystallization having the same profile of cooling was conducted and the oscillator was taken at the lowest coolant temperature for the microscopic observation of the crystals formed. Figure 3 illustrates the crystals from slow cooling of run-1. The intrinsic crystal shape of potassium nitrate is orthorhombic (aragonite), and the SEM photograph of slow cooling crystallization shows the shape. However, the fast cooling crystallization produces a different shape of product.

The measurement of resonant frequency using a quartz crystal oscillator indicates the difference of crystal growth rate, which can be used to predict the shape of crystallization product. In Table 1, the frequency decreasing rate is given to show the difference of crystal shape. While the slow cooling leads to a rate of 114 Hz/min, the fast does to a rate of 176 Hz/min. Therefore, the crystal shape can be predicted by monitoring the frequency variation of a quartz crystal oscillator in cooling crystallization.

The same procedure of the cooling crystallization and monitoring explained above was implemented to cupric sulfate solution. The monitoring results of resonant frequency and resistance along with temperatures of salt solution and coolant are shown, which demonstrate crystallization process for slow and fast cooling, respectively. The cooling rates and frequency decreasing rates are summarized in Table 1. As explained above, the slow cooling leaves the intrinsic shape of triclinic crystals demonstrated, whereas acicular crystals formed from fast crystallization are shown. The frequency decreasing rate indicates the difference of crystal shapes, which again proves that the monitoring the frequency variation can predict the shape of crystallization product.

In a practical application of the proposed device of crystal shape prediction, the manipulation scheme of solution temperature for a desired crystal shape can be obtained from the result of the prediction. Otherwise, the experimental operation has to be carried out to get the information in the field, which requires a significant amount of time and expense.

CONCLUSION

A monitoring system to predict the crystal shape from cooling crystallization was proposed and utilized to the crystallization of potassium nitrate and cupric sulfate solutions. The system was composed of a measurement device using a quartz crystal oscillator and an in-line solution flow and coolant flow systems. By applying two different cooling rates, different shapes of crystallization product were yielded while the resonant frequency variation was monitored to compare with the microscopic observation of the crystals formed. The experimental results indicate that the proposed monitoring system can effectively predict the crystal shape produced from practical crystallization processes.

ACKNOWLEDGMENT

Financial support from the Ministry of Commerce, Industry and Energy of Korea through the CANSMC is gratefully acknowledged.

REFERENCES

1. Joung, O. J., Kim, Y. H. and Fukui, K., "Determination of metastable zone width in cooling crystallization with a quartz crystal sensor," *Sens. Actuat. B:Chem.*, **105**, 464-472 (2005).
2. Joung, O. J., Kim, Y. H., Maeda, K. and Fukui, K., "Measurement of hysteresis in crystallization with a quartz crystal sensor," *Korean J. Chem. Eng.*, **22**, 99-102 (2005).
3. Kim, B. C., Kim, Y. H. and Fukui, K., "Crystallization monitoring in supersaturated solution with a quartz crystal sensor," *Anal. Chim. Acta*, **491**, 71-80 (2003).

Table 1. List of cooling rate and frequency decreasing rate.

Run	salt	cooling rate (°C/min)	frequency drop (Hz/min)	crystal shape
1	KNO ₃	0.11	114	orthorhombic (aragonite)
2	KNO ₃	0.29	176	cubic
3	CuSO ₄	0.25	154	triclinic
4	CuSO ₄	0.31	183	acicular

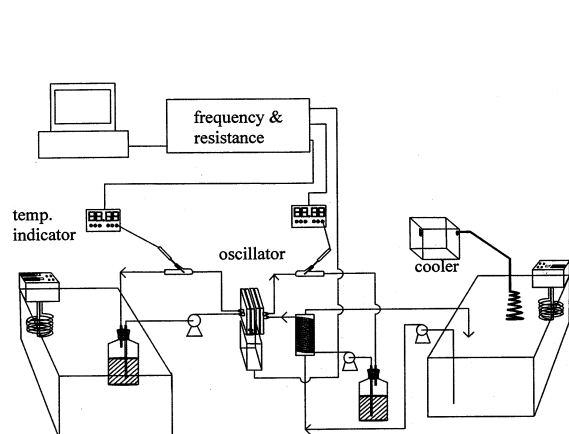


Fig. 1. A schematic diagram of the experimental setup with liquid flows and electrical wiring.

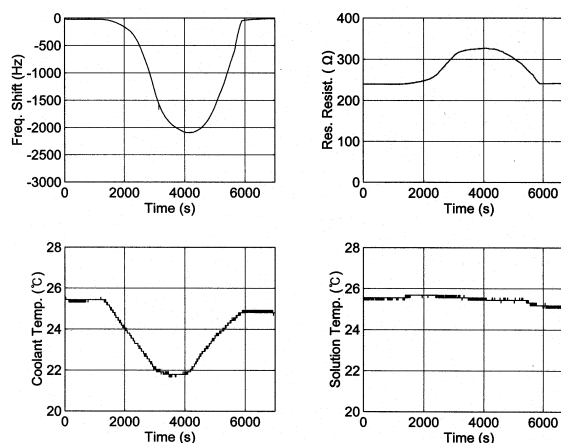


Fig. 2. Variations of resonant frequency and resistance, and coolant and solution temperatures in a slow cooling crystallization of potassium nitrate. (Run-1)

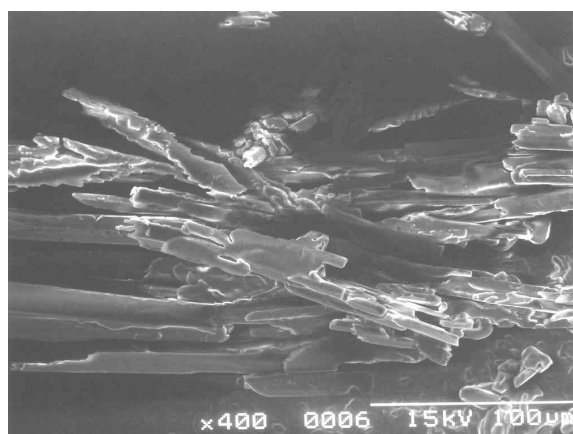


Fig. 3. A SEM photograph of orthorhombic crystalline formed from a slow cooling crystallization of potassium nitrate. (Run-1)